

## **OPERATING INSTRUCTIONS**

# DCX-22-CTD DATA LOGGER





➢ February 2022

## Table of contents


Product overview Overview of structural designs, Series DCX-22-CTD	3 4
Measuring principle for Series DCX-22-CTD	5
General	
Level measurement Relative pressure measurement (VG)	
Absolute pressure measurement (SG)	
Absolute/absolute pressure measurement (A/A)	
Level measurements in closed receptacles	
Functionality of the Series DCX-22-CTD	8
Data memory	
Installation instructions	9
Important information	
Guidelines on safe and efficient use	
Warranty conditions Data for repair and replacement	
Disposal of old electrical equipment and batteries / rechargeable batteries	
Fitting instructions	11
Requirements for the location	
Installation in level tubes	
Water level configuration	
Conductivity configuration	
Installation of relative data logger (VG versions)	
Configuring and reading the DCX-CTD	
DCX-CTD time Verifying measured data	
Device memory	
Maintenance	15
Battery	15
Changing the battery, Serie DCX-22-CTD	
Watertightness	
Ventilation diaphragm	
Moisture absorber cartridge	
Cleaning	17
Cleaning the level sensor	
Cleaning the air pressure sensor (AA versions)	
Calibration	18
Setting the zero point	
Testing by the manufacturer	10
Level measurement with pressure sensors	19 19
Converting conductivity measurements Overview of DCX-CTD	21
Accessories	23

## **Product overview**

The data loggers of the Series DCX-22-CTD are autonomous, battery-powered data collectors which can measure the water level (water column, i.e. pressure), conductivity and temperature over lengthy periods.

Series DCX-22-CTD is designed for level measurements and is generally used for longterm data acquisition in applications with brackish water, salt water or fresh water.

Various versions are available in Series DCX-22-CTD. The standard material is stainless steel, 316L (DIN 1.4435). For added resistance to media, the logger can be manufactured to order from Hastelloy or titanium as options. The key distinguishing features of products in Series DCX-22-CTD are their measuring methods.

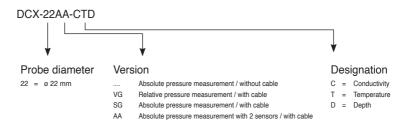


#### Maximum pressure ranges and cable lengths


Designation	Measuring principle	max. pressure range	max. electrical conductivity	max. mH2O	max. cable length**
DCX-22-CTD	absolute	0,811 bar abs.	0200 mS	0100 mH2O	-
DCX-22VG-CTD	relative	010 bar rel.	0200 mS	0100 mH2O	500 meters
DCX-22SG-CTD	absolute	0,811 bar abs.	0200 mS	0100 mH2O	500 meters
DCX-22AA-CTD	abs./abs.	0,811 bar abs.	0200 mS	0100 mH2O	80 meters

\*\* For other system lengths, please contact our sales staff

## Overview of structural designs, Series DCX-22-CTD

Different versions of the autonomous data logger Series DCX-22-CTD are available from KELLER in order to meet the requirements for the measuring point, the on-site environmental conditions and the fluid to be measured:

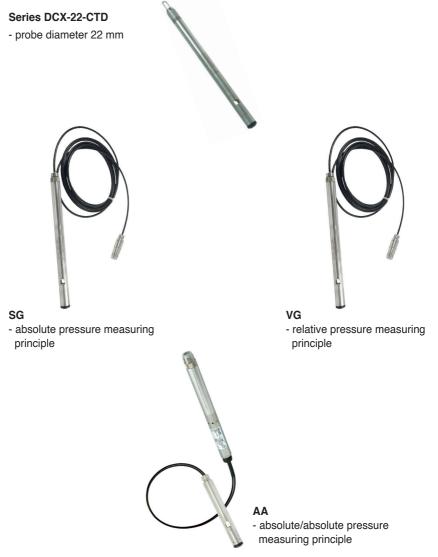

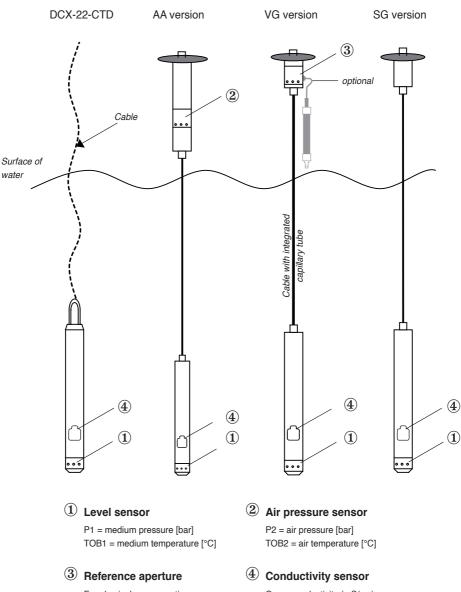

## Measuring principle for Series DCX-22-CTD

For physical compensation of the ambient pressure (air pressure)

## Con = conductivity (mS/cm)

T = medium temperature PT1000 (°C)

## **General information**

Fluctuations in the groundwater level (or the levels of other fluids) can be determined and located precisely by measuring the prevailing (hydrostatic) pressure at a defined depth below the surface of the water. To convert the pressure [bar] into the water column level [mH2O], it is only necessary to know the density of the fluid.

Example pure water (H2O): 100 mbar ≈ 1,02 mH2O

$$h = \frac{p}{\rho \cdot g} = \frac{N/m^2}{kg/m^3 \cdot m/s^2} = mH2O$$

p = hydrostatic pressure [Pa] (1 Pa = 1 N/m<sup>2</sup>, 0,1 bar = 10'000 N/m<sup>2</sup>)


 $\rho = \text{density} [\text{kg/m}^3]$ 

g = gravitational acceleration [m/s<sup>2</sup>]

h = height of water column [m]

#### Level measurement

In open systems, i.e. with the classical method of measuring the filling level, the difference between the pressure acting on the level sensor (total pressure) and the ambient pressure acting on the water (air/atmospheric pressure in most cases) is always measured. The pressure difference determined in this way corresponds to the hydrostatic water pressure.



As a result of this measurement method, the level measurement becomes independent of weather-induced fluctuations in air pressure that act on the surface of the fluid. The following methods of compensating for air pressure are available:

## Relative measurement method (VG)

In the relative measurement method, the sensor cable has an integrated capillary tube which provides the reference to the ambient air pressure directly on the level sensor. The sensor pressure measured in this way is therefore physically compensated for air pressure.

Advantage: high accuracy and resolution

Disadvantage: high ambient humidity at the measuring point may disrupt or interrupt compensation for air pressure and, in extreme cases, may even damage the level sensor (→ use moisture absorber cartridges)

## Absolute measurement method (SG)

With the absolute measurement method, the prevailing total pressure on the level sensor is determined (= air pressure + hydrostatic water pressure). To compensate for the influence of fluctuations in air pressure, a second data logger is positioned on the surface as a barometer.

Advantage: very robust, impervious to ambient humidity Disadvantage: no integrated air pressure compensation


## Absolute/absolute measurement method (AA)

Total pressure and air pressure are each determined by means of a pressure sensor (AA technology) and are calculated mathematically in the device by subtracting the two measured values. A sensor cable without a capillary tube is used for this measurement method, and this is why AA systems are highly resistant to the ambient humidity prevailing at the measuring point.

Advantage: very robust, impervious to humidity or flooding Disadvantage: slight reduction in measurement accuracy because of measurements by two sensors

## Level measurements in closed receptacles

For level measurement in closed receptacles/vessels, the internal pressure in the vessel is measured instead of the air pressure. The AA measurement method is usually selected on account of the humidity prevailing inside the vessel.



## Functionality of Series DCX-22-CTD

Autonomous data loggers in Series DCX-22-CTD record the values measured for pressure, conductivity and temperature together with the time of each measurement.

Recording interval	Constant storage interval	Interval ≥ 1 second		
	Event-controlled	If value is exceeded		
	recording	If value is undercut		
		If value changes		
Initial conditions	Directly after programmin	Directly after programming is completed		
	Specified, user-defined tin	Specified, user-defined time		
	Recording starts when a	Recording starts when a value has been undercut		
	Recording starts when a	Recording starts when a value has been exceeded		
$\rightarrow$ Constant storage interval and event-controlled recording can be used simultaneously				

The following types of recording and initial conditions are supported:

## Data memory

The following table gives an overview of recording periods for various constant measurement intervals (Data memory size 4 Mbit).

Please note the increased energy consumption and, therefore, the shorter battery life with frequent measurement intervals. Battery life: 10 years with 1 measurement per hour, 0,5 year with 1 measurement per minute, 10 days with 1 measurement per second (external influences can also reduce the battery life).

Туре	Interval	Number of channels	Measurement channel	max. data memory recording period
DCX-22-CTD	1 sec	2		> 15 h 54 min
DCX-22-CTD	1 min	2	Total pressure & conductivity	> 28 d 8 h
DCX-22-CTD	1 h	2		> 4 y 8 m
DCX-22-CTD	1 sec	3		> 6 h 36 min
DCX-22-CTD	1 min	3	Total pressure & medium tempe-	> 21 d 6 h
DCX-22-CTD	1 h	3	rature & conductivity	> 2 y 18 m
DCX-22-CTD	1 d	3		> 84 y 14 m
DCX-22AA-CTD	1 sec	6	Air pressure & air temperature, total	> 5 h 18 min
DCX-22AA-CTD	1 min	6	pressure & medium temperature, calculated water column level &	> 12 d 4 h
DCX-22AA-CTD	1h	6		> 2 y
DCX-22AA-CTD	1 d	6	conductivity	> 48 y 8 m

## Installation instructions

## Important information

## **KELLER** website

At www.keller-druck.com, you will find a «software», section where you can download all KELLER's software programs free of charge. The site contains the latest software versions together with datasheets and operating instructions for the corresponding products.

## Service and Support

For service and support, please contact your local dealer or contact us at www.keller-druck.com

## Guidelines on safe and efficient use

- Treat the product with care and keep it in a clean place that is free of dust.
- This product must only be used within the specified temperature range (→ Product datasheet).
- · Do not drop or throw the device.
- · Do not attempt to modify the device.
- Never damage or bend the conductivity sensor's metal rods.



• The sensor pressure diaphragm is sensitive to contact. Do not press the diaphragm in by hand or damage it with sharp objects. Do not direct water jets at the diaphragm.



 Only use this device for non-flammable fluids with no explosion hazard. KELLER offers a series of measurement equipment products suitable for use in areas with explosion hazards (ATEX zones). For more information, please contact our sales staff.



 Aggressive media may damage the product. Make sure that the materials in the product are not attacked by the medium to be measured.



• With relative versions (VG), the end of the cable must be located in a dry environment in order to prevent condensation forming. If the cable ends in a humid environment, it is highly advisable to use moisture absorber cartridges.



- The level measurement sensor must not freeze up in the medium.
- Do not glue, block or contaminate any ventilation components as this will substantially impair measurement accuracy.
- Fasten/secure the product so that the logger cannot fall into the measuring point in case of a handling error.

## Warranty conditions

The warranty does not apply to faults on the device caused by normal wear, incorrect use or misuse, or failure to comply with KELLER's instructions.

#### Data security

KELLER assumes no responsibility for data loss of any nature, and shall not pay compensatory damages in case of data loss. Data stored in the product may be lost if the product is repaired or replaced. You should always create a backup of all data stored in the product before releasing it for repair or replacement.

## Disposal of old electrical equipment and batteries



Do not dispose of batteries with general household waste. To prevent possible damage to the environment or to health due to uncontrolled waste disposal, this product must be separated from other waste and recycled correctly in order to ensure sustainable use of the raw materials.

## **Fitting instructions**



## **Requirements for the location**

The DCX-22-CTD logger unit is installed in a stable position at the measurement location.

- If the logger is fully sunk into the ground (e.g. in a sewer shaft), free movement of the water level in the tube must be ensured by above-ground openings (ventilation apertures).
- Lateral movements of the level sensor may cause measuring errors or cable breaks. For these reasons, fit the level sensor in a calm zone or in a suitable protective tube.
- On VG versions, the sensor cable contains a capillary tube to compensate for atmospheric pressure. Therefore, position the cable end of VG versions in a dry area or use moisture absorber cartridges



## Installation in level tubes

Place the cap lock in position and screw the two grub screws in to prevent it from turning (anti-theft protection)

→ requires a slotted screwdriver, size 2 (not included in the scope of delivery)



Guide the sensor with the sensor cable into the level tube by hand. The sensor cable must be free and extended as it hangs in the level tube; it must not change its position as this would falsify the measurement results. Align the DCX-22-CTD in such a way so as to ensure that the medium can flow through the flow opening of the sensor.

→ For system lengths of more than 50 m, cable strain relief is recommended, e.g. using a straining clamp (see Accessories)



Screw the matching adapter ring onto the read-out unit. After installation, the adapter ring will lie on the edge of the level cap lock. Secure the logger unit in the adapter ring using the circlip supplied with the product.

→ requires circlip pliers (not included in the scope of delivery)




The DCX-22-CTD logger can be connected locally to a laptop via the interface converter cable.

The KOLIBRI Desktop software can now be used to configure the device or to transmit the measurement data stored in the DCX-22-CTD to the laptop.



 $\rightarrow$  Seal the read-out plug with the protective cap



## Water level configuration

The surface of the interface plug integrated into the DCX-22-CTD represents the system's reference level. The measuring system is calibrated during installation. For this purpose, the run-off distance is measured (reference level-surface of water, e.g. using a light plummet) and is entered in the water level configuration in the KOLIBRI Desktop software together with the density of the medium. The system length is the sum of the hydrostatic water pressure measured at the level sensor and the distance from the reference level that is entered.

## Conductivity configuration

Before starting measurements, the conductivity sensor must be configured for the medium to be measured. This is carried out with the KOLIBRI Desktop software.Make sure that the probe is fully immersed in the medium and remove any trapped air inside the sensor element by carefully moving the measuring probe. Wait until the entire logger unit has reached the same temperature as the medium before starting long-term measurements.

#### Measuring range

Select the appropriate measuring range for your medium. In order to determine the appropriate measuring range, a preliminary measurement (online measurement) can be performed in the 200 mS/cm measuring range to determine the approximate conductivity.

#### **Temperature coefficient**

As well as the conductivity raw value, the logger unit also calculates the conductivity of the medium at 25 °C. As is the case with almost all physical processes, electrical conductivity is also temperature-dependent. The conductivity measurement can therefore be temperature-compensated to an agreed reference tem-perature – usually 25 °C – so that different measurements can be



compared. To do this, enter the temperature coefficient of the medium in the KOLIBRI Desktop software.

After completing work on the measuring point, close the level tube seal by screwing in the hexagon socket.

 $\rightarrow$  Allen wrench, size 5 (not included in the scope of delivery)

**Tip:** To give the measuring point better protection against access, the Allen screw head can be replaced by a screw head that is not available through usual commercial outlets.

## Installation of relative data logger (VG versions)

Ambient pressure is compensated physically on VG versions. The ambient pressure is fed to the back of the pressure sensor on the level sensor, via a capillary tube integrated into the sensor cable.

If pressure compensation via the capillary tube is impeded or prevented by contamination or moisture inside the capillary tube, the result of the level measurement will be affected.

## Standard version

The pressure compensation aperture is located behind the removable protective tube, which is perforated. This opening for the cable capillary is protected against water penetration by a Goretex<sup>®</sup> diaphragm.

A thread to insert moisture absorber cartridges is provided on the plug component of VG versions (minimum inner diameter of tube: ø 35 mm). It is advisable to use moisture absorber cartridges for measuring points with harsh ambient conditions.

→ section «Maintenance / Moisture absorber cartridge»



Moisture absorber cartridge



Version with moisture absorber cartridge

## Configuring and reading the data logger

The DCX-22-CTD is configured and read locally. The DCX-22-CTD is fitted in the measuring point and is connected to a laptop via the interface converter cable.

 The KELLER tutorials for the KOLIBRI Desktop software can be found at www.keller-druck.com

## Installing the software

Only connect the DCX-22-CTD and the converter cable to your computer after the software has been installed

- Install the KELLER «Driver K-114» software
- · Install the KELLER «KOLIBRI Desktop» software

## Maintenance

Dry the DCX-22-CTD thoroughly before opening it and make sure that the surrounding area is dry while handling the device. Check all the sealing rings for signs of wear, dirt and damage before using the logger unit again.

 $\rightarrow$  For spare parts, see Accessories

#### Battery

The battery status is not measured; instead, it is calculated using the averaged power consumption. If the battery is changed or in case of a «Power on» reset, the display is reset to 100 %. This also happens if the same battery is inserted again, or if a discharged battery is inserted.


To ensure that the logger operates reliably, it is advisable to replace the battery as soon as its capacity falls below 30 %, or after 5 years of operation.

## Changing the battery, Series DCX-22-CTD

Type designation	Supply	Battery type	KELLER product no.
DCX-22SG-CTD	Battery	Lithium battery (type AA)	557005.0006
DCX-22VG-CTD	Battery	Lithium battery (type AA)	557005.0006
DCX-22AA-CTD	Battery	Lithium battery (type AA)	557005.0006



Battery Series DCX-22-CTD Lithium battery (type AA) KELLER product no. 557005.0006

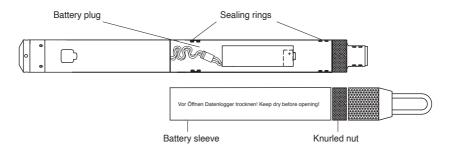

To replace the battery, first unscrew the knurled nut and then pull off the battery sleeve. Carefully disconnect the battery from the plug and replace it.

After changing the battery, guide the plug into the opening in the sleeve, push the battery in and fix it in the clip. Check the sealing rings. Re-fit the battery sleeve, knurled nut and fixture.

Check the configuration (time, measurement interval, etc.) of the DCX-22-CTD via the KOLIBRI Desktop software before using the product.

## Watertightness

Products in the Series DCX-22-CTD logger are dustproof and are protected against the effects of immersion in water (according to the pressure range).

The products are also protected against water splashes in the area of the read-out component.

Exceptions: AA products: may be flooded for brief periods DCX-22-CTD: continuous/long-lasting immersion

 $\rightarrow$  Please consult the datasheet for the precise specifications.

Check that all sealing rings are clean and undamaged, and that the battery compartment cover is firmly closed so that the Series DCX-22-CTD device is watertight.

## Ventilation diaphragm (for VG versions only)

The diaphragm used for ventilation generally requires no maintenance.

The ventilation function of the diaphragm is impaired by matter adhering to or contaminating the ventilation aperture, or by contact between the diaphragm and solvents, to such an extent that it may be necessary to replace the diaphragm. Test measurements are carried out to verify the pressure compensation function.

## Tip:


If blowing into the ventilation element during online measurements causes the value to change visibly, the ventilation diaphragm is in proper working order.

## Moisture absorber cartridges (optional)

The condition of the moisture absorber cartridge can be determined from the coloration of the granulate. Blue = granulate is dry, pink = granulate is moist.

The granulate can be regenerated for re-use. To do this, pour the granulate from the cartridge into a suitable container and dry it for 1 hour at 210 °C. The granulate releases moisture into the surrounding environment and takes on a blue color again. After drying, the granulate should be poured back into the absorber cartridge while it is still warm.

**Note:** The color of the granulate is less marked after regeneration than before because the indicator inside the granulate particles migrates.

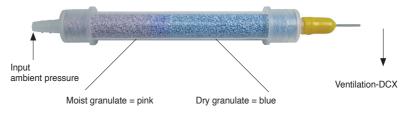

## Cleaning

If the data logger is used in severely contaminated media, the pressure sensor must be checked for contamination from time to time, and must be cleaned as necessary. Never use sharp-edged tools such as screwdrivers, and never apply pressure at any point on the diaphragm.

## Cleaning the level sensor

The protective cap over the pressure sensor on the level sensor can be removed by hand. Then rinse the sensor in flowing lukewarm water.

The pressure sensor diaphragm is very sensitive. **Do not touch the diaphragm!** 



## Cleaning the air pressure sensor (AA versions)

To clean the pressure sensor as thoroughly as possible, remove the knurled nut, battery sleeve and the protective sleeve of the sensor, and then re-install the battery sleeve, the protective cap for the interface plug and the knurled nut (without the protective sleeve for the sensor) so that the electronics are protected against water and moisture.

Rinse the sensor with clean lukewarm water. After cleaning and before fitting the sleeves, make sure that all parts are dry.

The pressure sensor diaphragm is very sensitive. **Do not touch the diaphragm!** 

## Cleaning the conductivity sensor

Clean the conductivity probe with soapy water and cotton buds. Any deposits on the conductivity sensor can be removed using a water and vinegar solution. Next, rinse the conductivity probe thoroughly with water. Never bend or modify the sensor element's metal rods.



Plug for converter cable



Calibration

## Setting the zero point

The pressure sensors built into the logger unit can be calibrated by the user. It may be necessary to recalibrate the pressure sensors, for example after maintenance work, if the measurement set-up is changed, or after the measuring station has been operated for a year or more.

Calibration is carried out with the KOLIBRI Desktop software. Recommended interval between calibrations: 1–2 years.

When carrying out a calibration, note that the sensors must be checked/calibrated in the same positions as they occupy in the measuring point (usually upright) and they must be positioned next to each other at the same level.

## Calibrating the conductivity sensor

The calibration is carried out with the KOLIBRI Desktop software. Recommended interval between calibrations: calibration only as required.

Data logger

## Testing by the manufacturer

The DCX-22-CTD may also be sent to KELLER AG für Druckmesstechnik in order to verify its measurement accuracy or for calibration. The following test options may be chosen: simple check on the DCX-22-CTD without documentation, internal check with documentation (5- or 11-point test protocol) or an internal check followed by external certification (DKD [German Calibration Service] or SCS [Swiss Calibration Service] calibration certificate).

(Charges are payable for checks/verifications, calibrations, protocols and certificates)

## Level measurement with pressure sensors

Series DCX-22-CTD devices measure and store the hydrostatic pressure of a fluid in bar. The density of the medium has a decisive influence on the conversion of the pressure [bar] to the water column level [mH2O]. The height of the water column is calculated with the following formula in the KOLIBRI Desktop software:

h = 
$$\frac{p}{\rho \star g}$$
 =  $\frac{10000 \text{ N/m}^2}{998,207 \text{ kg/m}^3 \star 9,80665 \text{ m/s}^2}$  = **1,021 mH2O**

p = hydrostatic pressure [Pa] (1 Pa = 1 N/m<sup>2</sup>, 0,1 bar = 10'000 N/m<sup>2</sup>)

 $\rho$  = water density [kg/m<sup>3</sup>] = 998,207 kg/m<sup>3</sup> @ 20 °C

g = gravitational acceleration [m/s<sup>3</sup>] (= 9,80665 m/s<sup>2</sup>)

h = height of water column [m]

## **Converting conductivity measurements**

## Conductivity $[\gamma]$ of the measured medium

The DCX-22-CTD series measures the electrical conductivity at the current temperature in mS/cm and stores the result. As is the case with almost all physical processes, electrical conductivity is also temperature-dependent. It is therefore important to adjust the measurements to an agreed reference temperature – usually 25  $^{\circ}$ C – so that different measurements can be compared. The following formula is used to convert the measurement to electrical conductivity at 25  $^{\circ}$ C (in accordance with ISO7888 / EN 27888):


 $\gamma_{25} = \frac{\gamma_{\Theta}}{1 + (\alpha/100) (\Theta-25)}$ 

- $\alpha$  = Temperature coefficient of the electrical conductivity
- $\gamma_{\scriptscriptstyle \Theta}$  = Electrical conductivity at measurement temperature  $\Theta$
- Θ = Measurement temperature of the sample in °C

You can use your own formulae to calculate the compensated conductivity from the conductivity raw value by exporting the data from the measurement file, e.g. into Microsoft Excel.

#### Density [p] of the measured medium

The density of fluids is temperature dependent. The density of most fluids decreases in linear proportion to the temperature. However, water reaches its highest density at 3,98 °C; above and below this temperature, the density of water decreases. This phenomenon is also referred to as the «density anomaly of water».



Make sure that the correct density of the measured medium is entered in the KOLIBRI Desktop software in order to calculate the level.


The density entered in the KOLIBRI Desktop software is static. Changes in the temperature of the measured medium and the associated change in density are not taken into account when calculating the water level because this could result in misinterpretations of the measurement result on account of the heterogeneous temperature distribution in bodies of still water.

In normal cases, the temperature distribution is heterogeneous, so the temperature dependency can be neglected. In case of homogeneous temperature distribution and major temperature changes, however, a conversion error between pressure [bar] and level [mH2O] occurs due to the density that is stored as a static value.


Temp. [°C]	Pressure [bar]	Density [kg/m <sup>3</sup> ]	Calculated water level	Error at 5 mH2O [cm]
4	0,5	999,975	5,0987 m	0 cm
10	0,5	999,702	5,1001 m	+ 0,14 cm
15	0,5	999,103	5,1032 m	+ 0,45 cm
20	0,5	998,207	5,1077 m	+ 0,9 cm
25	0,5	997,048	5,1137 m	+ 1,5 cm
30	0,5	995,65	5,1209 m	+ 2,22 cm

(Water, temperature range 0...30 °C, pn = 1013 kPA).

## **DCX-CTD** overview

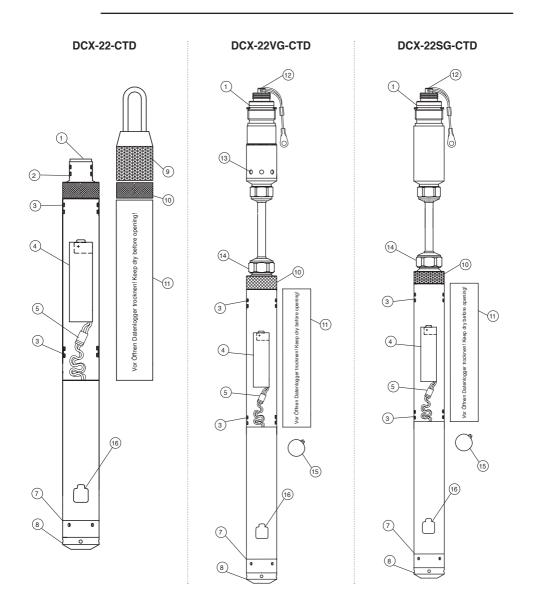

## DCX-22AA-CTD

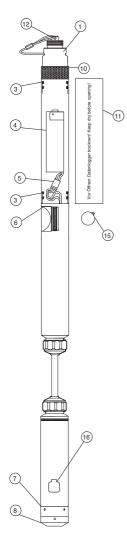

Nr.	Designation
1	Interface plug RS485 with protective cap
2	Sealing ring for interface plug
3	Sealing ring for battery compartment
4	AA lithium battery
5	Battery plug
6	Air pressure sensor
7	Sensor reference line
8	End cap
9	Fixture with hook to secure the suspended cable
10	Knurled nut
11	Battery sleeve
12	Cap lock for interface plug
13	Ventilation aperture (only present on VG versions)
14	Screw nut
15	Circlip
16	Conductivity sensor

KELLER product numbers are shown in the list of accessories (starting on page 23).

## Accessories

DESCRIPTION	SCOPE OF DELIVERY	PRO	DUCT	NO.	
Software CD Contains all KELLER software including USB driver for K-114 Can be downloaded free of charge at: www.keller-druck.com	Supplied with product	7505	05.00	KELL	LER Software CD may No. 70055 0001 ketter druck com
Adapter rings for DCX (can be supplied as an option)	Optional				 9 mm ↓
Suitable for - DCX-22-CTD		sic	y           25           25           39           50           55           32           32	<b>v</b> <b>Drawing no.</b> 33386 Pos. 1 33386 Pos. 2 33386 Pos. 4 33386 Pos. 4 33386 Pos. 5 33386 Pos. 6 33386 Pos. 8 33386 Pos. 9	Product no. 506810.0006 506810.0018 506810.0015 506810.0019 506810.0014 506810.0020 506810.0022 506810.0025
		42 76 125	32 32 32	33386 Pos. 10 33386 Pos. 11 33386 Pos. 12	506810.0026 506810.0027 506810.0030
Cap lock, DCX 2" 3" 4" 5" 6"	Optional	5068 5068 5068	15.00( 15.004 15.004 15.004 15.004	40 41 42	

DESCRIPTION	SCOPE OF DELIVERY	PRODUCT NO.
Adapter ring to match DCX cap lock 3" 4" 5" 6" → to install the DCX-CTD logger in the level tube, an adapter ring (2" pot) is	Optional	506810.0085 506810.0085 506810.0087 506810.0078
required		
Adapterring 2" Pott	Optional	506810.0021
End cap	Supplied with product	507220.0001
Protective cap with filter	Optional	507220.0002
Battery to match: DCX-22 (AA/SG/VG) / CTD	Supplied with product	557005.0006

DESCRIPTION	SCOPE OF DELIVERY	PRODUCT NO.
Flange socket for connection socket with hexagon socket screw (Inox M3 x 6) for securing	Supplied with product for DCX-22AA-CTD SG-CTD VG-CTD	508415.0004
<b>Circlip</b> DIN: 471 (BN: 682) ø 18 mm	Supplied with product for AA/VG/SG versions	508830.0002
O-ring, interface plug ø 13 mm x 1,5 mm / Nitrile	Spare part	508610.0051
O-Ring Batteriefach ø 17 mm x 1,5 mm / Nitrile	Spare part	508610.0024

DESCRIPTION	SCOPE OF DELIVERY	PRODUCT NO.
Interface converter K-103A For communication between PC and DCX-22-CTD. Connection to serial interface (converter RS232 – RS485)	Optional	309010.0002
Interface converter K-114A with Fischer plug/ 5-pin: • Supply via USB for a connected end consumer (U-Out = 11,8 VDC / I-Out <sub>max</sub> = 40 mA) • Optical status and configuration display (LED) • Electrical isolation • Total length: 1,7 m • Software CD and USB connection cable included in scope of delivery	Optional	309010.0075

KELLER AG für Druckmesstechnik St. Gallerstrasse 119 • CH-8404 Winterthur Tel. +41 52 235 25 25 • Fax +41 52 235 25 00

www.keller-druck.com



